


**USP 467 Procedure B - Class 1 by GC/FID on ZB-WAXplus****Column:** Zebtron<sup>™</sup> ZB-WAXplus<sup>™</sup>, GC Cap. Column 30 m x 0.32 mm x 0.25 µm, Ea**Phase:** Polyethylene Glycol (PEG)**Dimensions:** 30 meters x 0.32 mm x 0.25 µm**Order No:** 7HM-G013-11**Oven Profile:****Carrier Gas:** Constant Flow Helium, 35 cm/sec**Injection:** Headspace 5.000000000:1 0 µL @ 140°C**Detection:** Refractive Index (250°C)**Analyst Note:** Sample prepared as per USP Method**Products used in this application:****ANALYTES:**

- 1 1,1-Dichloroethene
- 2 Carbon tetrachloride
- 3 1,1,1-Trichloroethane
- 4 Benzene
- 5 1,2-Dichloroethane

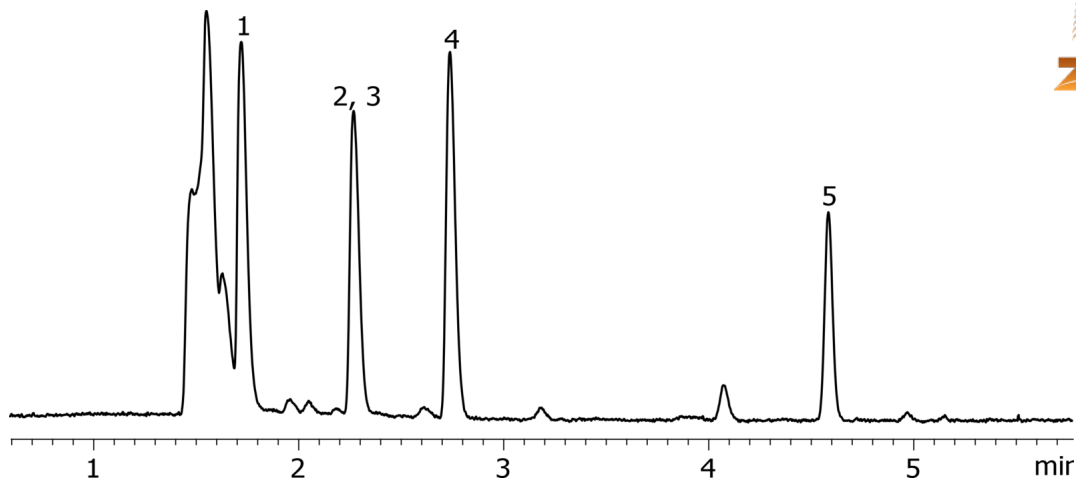