

Performance Comparison: Aeris PEPTIDE 3.6u XB-C18 vs Acquity (vs19930) for Hu Ig-G digest

Column: Aeris™ 3.6 µm PEPTIDE XB-C18 100 Å, LC Column 150 x 2.1 mm, Ea

Dimensions: 150 x 2.1 mm ID

Order No: 00F-4507-AN

Elution Type: Gradient

Eluent A: Water with 0.1% TFA

Eluent B: Acetonitrile with 0.1% TFA

Gradient Profile:	Step No.	Time (min)	Pct A	Pct B
	1	0	97	3
	2	5	97	3
	3	60	55	45

Flow Rate: 0.3 mL/min


Col. Temp.: 40 °C

Detection: Circular Dichroism @ 0.0000000000 (ambient)

Analyst Note: SecurityGuard™ Guard Cartridge System extends column lifetime.

- SecurityGuard ULTRA Cartridges, UHPLC C18-Peptide for 2.1mm ID Columns, 3/Pk Part No.: AJ0-8948


- Holder Part No.: AJ0-9000



Products used in this application:



19928

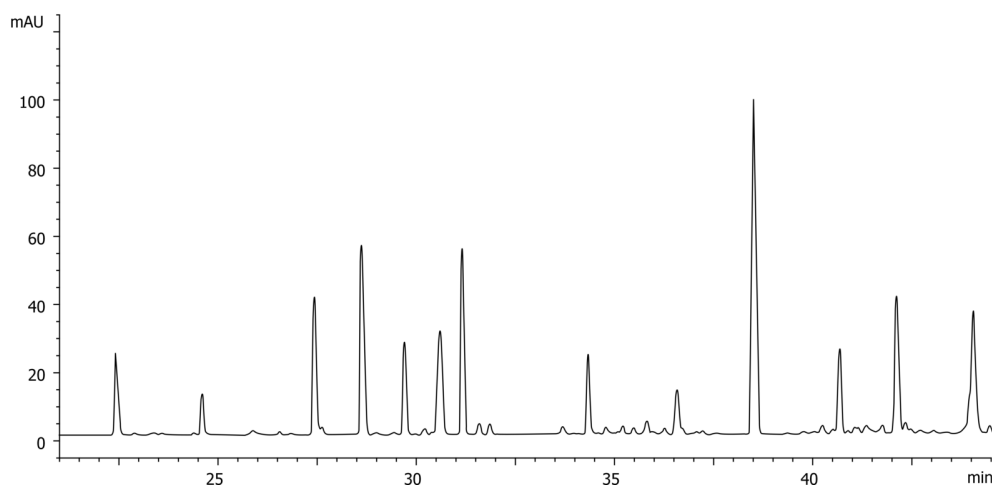

ANALYTES:

1 Human IgG

