

Aldosterone on Kinetex 2.6 µm XB-C18 50x3 mm ID

Column: Kinetex® 2.6 µm XB-C18 100 Å, LC Column 50 x 3 mm, Ea

Dimensions: 50 x 3 mm ID

Order No: 00B-4496-Y0

Elution Type: Gradient

Eluent A: DI Water

Eluent B: Methanol/Acetonitrile (50:50)

Gradient Profile:	Step No.	Time (min)	Pct A	Pct B
	1	0	70	30
	2	4	10	90
	3	5	10	90
	4	5.1	70	30
	5	7	70	30

Flow Rate: 500

Col. Temp.: ambient


Detection: Circular Dichroism @ 0.0000000000 (ambient)

Analyst Note: SecurityGuard™ ULTRA Guard Cartridge System extends column lifetime.

- SecurityGuard ULTRA Cartridges, UHPLC C18 for 3.0mm ID Columns, 3/Pk Part No.: AJ0-8775

- Holder Part No.: AJ0-9000

20009

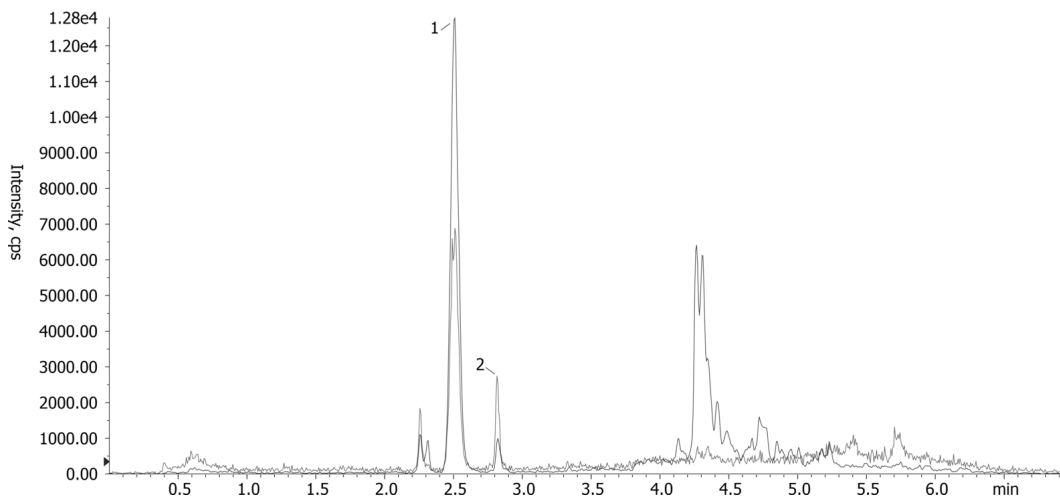

ANALYTES:

1 Aldosterone

Retention Time: 2.52 min

2 Cortisone

Retention Time: 2.84 min



Products used in this application:



Sample Preparation Details

for HPLC Application ID No.: 20009

Aldosterone on Kinetex 2.6 μ m XB-C18 50x3 mm ID

PRODUCT DESCRIPTION:

StrataTM-X-A 33 μ m Polymeric Strong Anion, 60 mg / 3 mL, Tubes , 50/Pk

Order No.: 8B-S123-UBJ

SOLID PHASE EXTRACTION (SPE) PROCEDURE:

Note: The solvent volumes shown below are for a 60 mg bed mass.

The solvent volumes will need to be adjusted for a smaller or larger bed mass.

Condition:

Load:

Wash:

Dry:

5 min at high vacuum

Elute:

Final Prep and Analysis:

Inject: 0 μ L on HPLC Circular Dichroism @ 0.0000000000 (ambient)

ANALYTES:	Spiked Conc. (ng/mL)	Log P	pKa	% Rec	%RSC (n=0)
1 Aldosterone	0				
2 Cortisone	0				

Note: This method is designed as a convenient starting point for further investigation and can be tailored to meet your extraction goals.
Call your local Phenomenex Representative for assistance in method development and optimization techniques.

©2025 Phenomenex Inc. All rights reserved.

For more information contact your Phenomenex Representative at support@phenomenex.com



Phenomenex products are available worldwide.

www.phenomenex.com

support@phenomenex.com