


Degraded Human Insulin on Yarra 1.8 µm SEC-X150

Column: N/A
Dimensions: N/A
Order No: N/A
Elution Type: N/A
Eluent A: 1g/L L-Arginine in water
Eluent B: Acidic Acid
Eluent C: Acetonitrile
Gradient Profile:

Step No.	Time (min)	Pct A	Pct B	Pct C
1	0	65	15	20

Flow Rate: 0.2 mL/min
Col. Temp.: ambient
Detection: Electrospray Mass Spec (ESMS) @ 0.0000000000 (ambient)

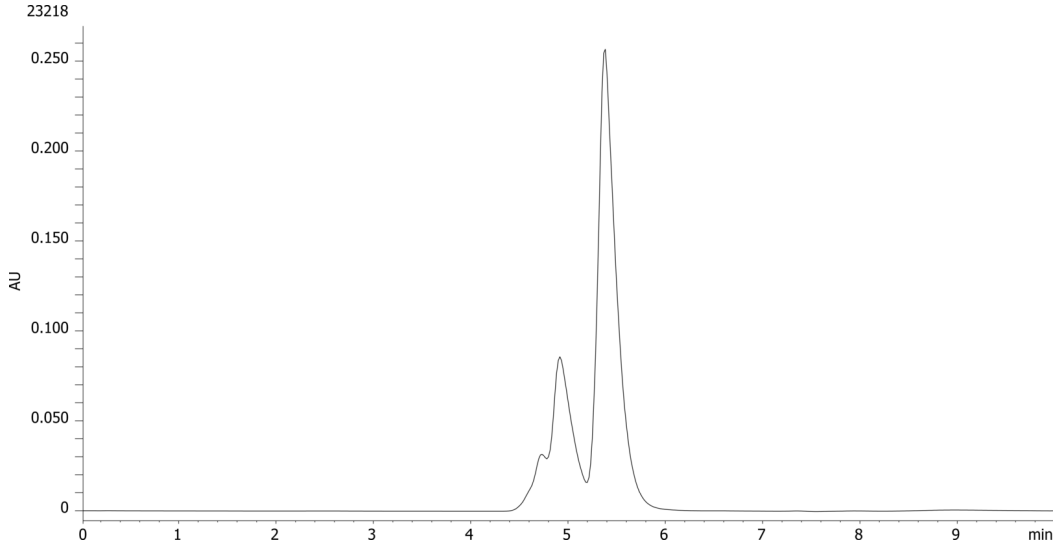

ANALYTES:

- 1 Aggregates
Retention Time: 4.735 min
- 2 Aggregates
Retention Time: 4.919 min
- 3 Insulin
Retention Time: 5.38 min

