

HPLC Application

ID No.: 27882

USP Tigecycline Assay Standard Solution on Luna 5u C18(2) 150x4.6mm using Agilent 1260 Quaternary UHPLC s

Column: Luna® 5 µm C18(2) 100 Å, LC Column 150 x 4.6 mm, Ea

Dimensions: 150 x 4.6 mm ID

Order No: 00F-4252-E0

Elution Type: Isocratic

Eluent A: Acetonitrile:Buffer (140:860) Buffer: 4.35g/L of dibasic Potassium Phosphate and 0.93 g/

Gradient

Step No.	Time (min)	Pct A
1	45	100

Profile:

Flow Rate: 1 mL/min


Col. Temp.: 30 °C

Detection: UV-Vis Abs.-Diode Array (PDA) @ 248.000000000 nm (nanometers) (ambient)



Phosphori

Products used in this application:

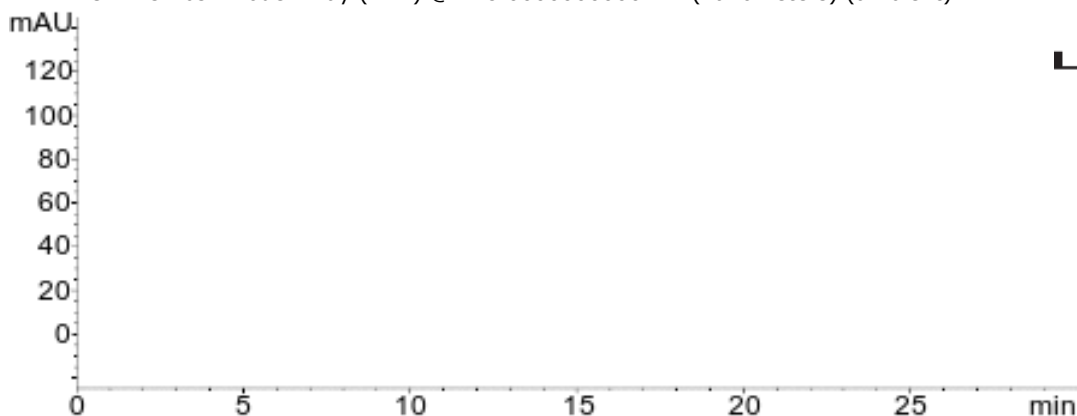

ANALYTES:

1 Tigecycline

Retention Time: 12.758 min

